
Cell-free layer analysis in a polydimethylsiloxane microchannel: a global approach

Elmano Pinto, Vera Faustino, Diana Pinho,
Raquel O. Rodrigues, Rui A. Lima and
Ana I. Pereira*

Polytechnic Institute of Bragança, ESTiG/IPB,
C. Sta. Apolónia, 5301-857 Bragança, Portugal
and

ALGORITMI, University of Minho, Guimarães,
Campus Azurém, 4800-058 Guimarães, Portugal

Email: elmano@ipb.pt

Email: verafaustino@ipb.pt

Email: diana@ipb.pt

Email: raquel.rodrigues@ipb.pt

Email: rl@dem.uminho.pt

Email: apereira@ipb.pt

*Corresponding author

Abstract: The cell-free layer (CFL) is a hemodynamic phenomenon that has an important contribution to the rheological properties of blood flowing in microvessels. The present work aims to find the closest function describing RBCs flowing around the cell depleted layer in a polydimethylsiloxane (PDMS) microchannel with a diverging and a converging bifurcation. The flow behaviour of the CFL was investigated by using a high-speed video microscopy system where special attention was devoted to its behaviour before the bifurcation and after the confluence of the microchannel. The numerical data was first obtained by using a manual tracking plugin and then analysed using the genetic algorithm approach. The results show that for the majority of the cases the function that more closely resembles the CFL boundary is the sum of trigonometric functions.

Keywords: red blood cells; RBCs; cell-free layer; CFL; nonlinear optimisation; global optimisation.

Reference to this paper should be made as follows: Pinto, E., Faustino, V., Pinho, D., Rodrigues, R.O., Lima, R.A. and Pereira, A.I. (2016) 'Cell-free layer analysis in a polydimethylsiloxane microchannel: a global approach', *Int. J. Medical Engineering and Informatics*, Vol. 8, No. 3, pp.196–209.

Biographical notes: Elmano Pinto received his BS in Biomedical Engineering from the Polytechnic Institute of Bragança in 2010, and his MS in Biomedical Technologies from the Polytechnic Institute of Bragança in 2012.

Vera Faustino received her BS in Biomechanics from the Polytechnic Institute of Leiria in 2009, and her MS in Biomedical Technologies from the Polytechnic Institute of Bragança in 2012. Currently, she is a PhD student of Biomedical Engineering at Minho University. Her areas of interest are microfluidics, microfabrication, separation of cells and particles.

Diana Pinho received her BS in Biomedical Engineering from the Polytechnic Institute of Bragança in 2010, and her MS in Biomedical Technologies from the Polytechnic Institute of Bragança in 2011. Currently, she is a PhD student of Mechanical Engineering at Porto University. Her areas of interest are blood and blood analogues rheology, microfluidics, microfabrication and cell-free layer development microchannels.

Raquel O. Rodrigues received her BS in Biotechnology Engineering from the Polytechnic Institute of Bragança in 2007, and her MS in Biomedical Technologies, in 2012, from the Polytechnic Institute of Bragança. Since September 2014, she is a PhD student, with a grant of FCT, in Chemical and Biological Engineering at Porto University. Currently, her work is focused in the development of magnetic nanoparticles for hyperthermia treatment and also in the study of their transport in the blood stream using microfluidic devices.

Rui A. Lima is an Assistant Professor at the Department of Mechanical Engineering, University of Minho (UM), a Research Fellow at the Transport Phenomena Research Center (CEFT), FEUP, University of Porto and an external collaborator at the Polytechnic Institute of Bragança (IPB). He received his PhD in Engineering (2007) from Tohoku University, Japan and PhD in Biomedical Engineering (equivalence, 2008) from Minho University.

Ana I. Pereira is an Assistant Professor at the Department of Mathematics, Polytechnic Institute of Bragança, and she is a member of the Algorithm Research Centre – Minho University. She received her PhD at Minho University (2006) in Numerical Optimisation area with the thesis ‘A reduction method to solve semi-infinite programming problems’. She is the author or co-author of more than 40 journal papers, book chapters and conference proceedings.

1 Introduction

Blood is a complex fluid composed mainly of suspended red blood cells (RBCs) within plasma where RBCs are responsible for the supply of oxygen and nutrients to the body and removal of carbon dioxide and metabolic wastes from tissues. Throughout the years, several experimental methods were performed in both *in vivo* (Maeda, 1996; Pries and Secomb, 1994; Suzuki et al., 1996; Kim et al., 2009) and *in vitro* (Faustino et al., 2014; Goldsmith and Turitto, 1986; Lima et al., 2006, 2008, 2009a, 2009b; Rodrigues et al., 2014) environments, in an attempt to understand the flow behaviour of RBCs in microchannels and microvessels. These studies have produced significant findings on the blood rheological properties at a micro-scale level. A hemodynamic phenomenon observed in both *in vivo* and *in vitro* studies is the formation of a marginal cell-free layer (CFL) at regions adjacent to wall due to the tendency of RBCs to migrate toward the centre of the microtube (Caro et al., 1978; Garcia et al., 2012; Maeda, 1996). The existence of a cell depleted layer in microvessels, tend to reduce the apparent viscosity of blood and by increasing this layer the blood viscosity tend to decrease in both microchannels and microvessels. Hence, it is important to understand the behaviour of the CFL in microcirculation as it contributes to the rheological properties of blood flowing in microvessels, modulates the nitric oxide scavenging effects by RBCs and may lead to heterogeneous distribution of blood cells in microvascular networks (Fedosov et

al., 2010; Kim et al., 2009). Additionally, several research studies have developed microfluidic systems able to perform blood separation using the advantage of the CFL formation in PDMS microchannels with dimensions smaller than 300 μm . Faivre et al. (2006), Sollier et al. (2010), Yaginuma et al. (2013) and Pinho et al. (2013b) have demonstrated that the presence of a constriction increases the CFL and as a result they were able to perform the separation of RBCs from plasma. Therefore, it is also important to improve our understanding regarding the CFL phenomenon happening in constriction geometries in order to improve the performance of blood separation microfluidic devices.

Although *in vivo* and *in vitro* experiments gives more realistic information on the flow properties of blood, once validated, physical models and their numerical results are extremely valuable tools to obtain more insight on the blood rheological properties at a micro-scale level. Recently due to the advances of the computational techniques and computing power, several numerical models have been proposed based on a multiphase approach, in which the blood is considered as a multiphase suspension of deformable particles and where levels of submodelling for the blood cells behaviour are also taken into account. Some examples for this type of approach are the boundary element method (Omori et al., 2011), the immersed boundary method (Bagchi, 2007; Eggleton and Popel, 1998), the lattice Boltzmann method (Dupin et al. 2007) the dissipative particle dynamics method (Fedosov et al., 2010), the moving particle semi-implicit (MPS) method (Imai et al., 2010; Tsubota et al., 2006a, 2006b; Gambaruto, 2015) and spring-network model based on the minimum energy concept (Lima et al., 2009a, 2009b; Nakamura et al., 2013). Reviews on these numerical methods can be found at Liu et al. (2006), Yamaguchi et al. (2006) and Lima et al. (2012). Although multiphase approaches are promising methods, it is still extremely complex to consider the CFL in their numerical models, so optimisation can be also an important field of study to help in the development of numerical simulations. In recent years, optimisation algorithms have become increasingly robust and as a result several researchers have applied this methodology to study phenomena happening in microfluidic devices. For instance, Bento et al. (2015) have measured the CFL in a network containing multiple bifurcations and confluences and they have shown that the function that best fits the CFL was the sum of trigonometric functions.

The present study tracks RBCs flowing around the CFL and calculates the most suitable function by using global optimisation technique. The measurements were performed in a polydimethylsiloxane (PDMS) microchannel with a diverging and a converging bifurcation and all images were obtained by means of a high-speed video microscopy system.

The paper is organised as follows. Second section shows the materials used in this work and the methods that were applied in this study. The third section presents the numerical results and discussion. The last section presents the main conclusions and some future directions.


2 Materials and methods

2.1 Microchannel geometry

Microchannels were initially developed with a CAD software, where the geometries were selected taking into account a previous study about the blood flowing through

microchannels with bifurcations and confluences fabricated by a soft lithography technique (Leble et al., 2011). In this study, the parent microchannels have a width of 300, 500 and 1,000 μm and the two branches of the bifurcation and confluence correspond to 50% of the parent microchannel width. Figure 1 shows the configuration of the network and the regions where the CFL was measured, where RA and RB are the upper regions of the microchannel and RC and RD are the lower regions.

Figure 1 Schematic representation of the microchannel geometry and location of the sections where the images were collected and the CFL was measured

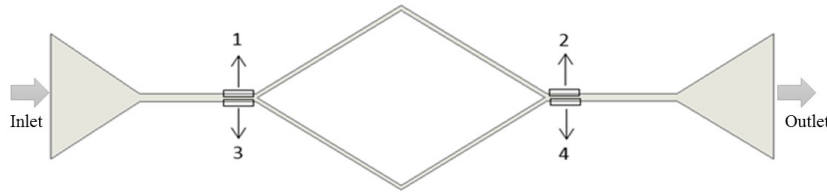

Notes: 1 – Region A ($R_{A(\text{width})}$); 2 – Region B ($R_{B(\text{width})}$); 3 – Region C ($R_{C(\text{width})}$) and 4 – Region D ($R_{D(\text{width})}$).


This geometry was used to fabricate the vinyl master moulds by using a soft xurography technique (Pinto et al., 2015). The moulds were used for the production of PDMS microchannels. Briefly, the PDMS was obtained by mixing a curing agent (10:1 ratio) with PDMS prepolymer. By using a spin coater, a residual amount of PDMS with a ratio 20:1 was dispersed on a slide glass. The PDMS was cured in an oven at 80°C for 20 minutes. Then, by using a blade the microchannels were cut off and the inlet/outlet holes were done by using a fluid dispensing tip. Finally, to have a strong adhesion of the materials, the device was placed in the oven at 80°C for 24 hours. More detailed information about this process can be found at Pinto et al. (2015).

2.2 Working fluids and experimental set-up

The fabricated microchannels were used to study *in vitro* blood flow with Dextran 40 containing 10% of RBCs. The blood was collected from a healthy sheep and heparin was added to prevent clotting. Additionally, the cells were separated from blood by centrifugation.

A syringe pump (Harvard Apparatus PHD ULTRATM) was used to control the flow rate of the working fluid. To visualise and measure the flow we have used an inverted microscope (IX71, Olympus) combined with a high-speed camera (i-SPEED LT). Figure 2 shows the experimental apparatus used to control the flow and to visualise the CFL within the microchannels. The microfluidic device containing the microchannels was placed on the stage of the inverted microscope and a pressure-driven flow was kept constant by means of a syringe pump. All images have a resolution of 800×600 pixels and were recorded at a frame rate of 200 frames/s.


Figure 2 Experimental apparatus to control and visualise the flow in microchannels produced by xurography (see online version for colours)

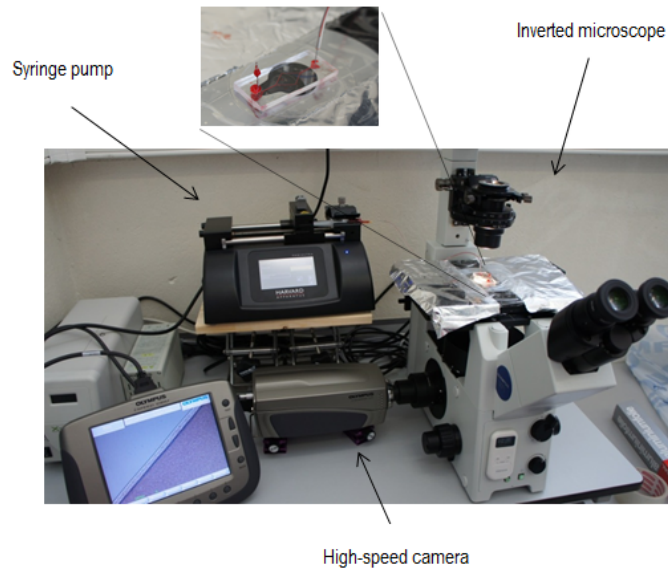

2.3 Image analysis

A manual tracking plugin (MTrackJ), of the image analysis software Image J (NIH), was used to track individual RBC flowing around the boundary of the RBCs core. By using MTrackJ plugin, the centroid of the selected RBC was automatically computed. After obtaining x and y coordinates of the RBC centroids, the data were exported for the determination of each individual RBC trajectory (Lima et al., 2008; Pinho et al., 2013a). Figure 3 shows a trajectory of a RBC flowing around the boundary region between the CFL and RBCs core.

Figure 3 A trajectory of a RBC flowing around the boundary region between the CFL and RBCs core (see online version for colours)

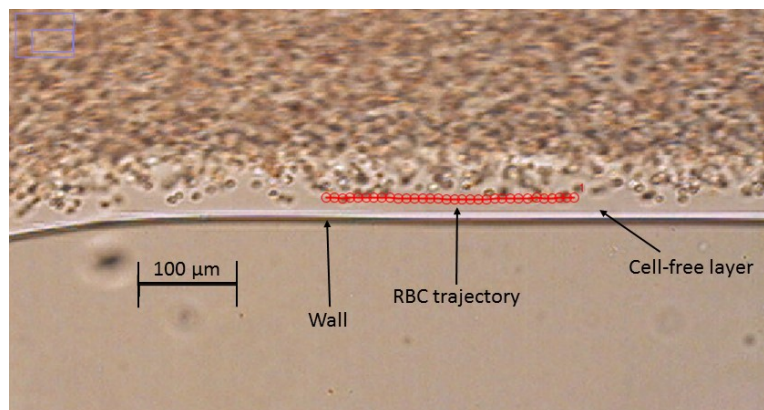

2.4 Global optimisation method: genetic algorithm

Genetic algorithms are based on theory of evolution of species from Darwin. This method allows to find a global minimum in a large search space (Holland, 1975). The genetic algorithm starts with a set of solutions called population, where the solution is represented by an individual and the population size is preserved through each generation. The objective function is evaluated in each individual. Then individuals are selected according to their objective value. Those selected will be reproduced up randomly, by using genetic operators such as mutation and crossover. Individuals with less value have a high probability of being selected whereas the new generation of individuals may have a minor objective value than the previous generation. The evolution process is repeated until the stopping criterion is satisfied (Bento et al., 2013, 2015; Catlin et al., 2011; Kumar et al., 2010). In this work it was implemented the genetic algorithm proposed by Bento et al. (2013, 2015) using Matlab software.

3 Results and discussion

All videos captured were recorded in four different regions, i.e., region RA and RC correspond to locations before the bifurcation whereas region RB and RD correspond to locations after the confluence (see Figure 1). Moreover, this study investigated the CFL behaviour in three kinds of parent microchannels having widths of 300, 500 and 1,000 μm . For all the cases, the flow rate was constant (10 $\mu\text{l}/\text{min}$) and the working fluid had always a hematocrit (Hct) of 10 %, i.e., containing 10 % of ovine RBCs in the solution. By using 10 % Hct we were able to track several individual RBCs. In fact 10% Hct is not far from the real Hct in microcirculation. It is known that, when the size of vessels becomes smaller the Hct tends to decrease. Additionally, dextran 40 was used to avoid the sedimentation of the cells.

A manual tracking plugin from Image J was used to track individual RBC flowing around the boundary region between the CFL and RBCs core. All the selected RBCs have good enough quality images to track the trajectory of the cells flowing nearby the RBCs core (see Figure 3). Figures 4, 5 and 6 show representative RBC trajectories in the different cases under study, i.e., parent microchannels with widths of 300, 500 and 1,000 μm at two different regions (region before the bifurcation and after the confluence).


To obtain the numerical data a nonlinear least squares theory was used. In each region R_{Aw} , R_{Bw} , R_{Cw} , and R_{Dw} for $w = 300, 500$ and $1,000$, we have applied the nonlinear optimisation problem defined as follows:

$$\begin{aligned} \min f(y) &= \sum_{k=1}^{N_R} (M_k - g_h(y, x_k))^2 \\ \text{s.t. } g_h(y, x_k) &\geq 0 \quad \forall k = 1, \dots, N_R \end{aligned} \quad (1)$$


where (x_k, M_k) , for $k = 1, \dots, N_R$ are the CFL measurement of region R (defined as R_{Aw} , R_{Bw} , R_{Cw} , and R_{Dw} for $w = 300, 500$ and $1,000$). The function g_h , for $h = 1, \dots, 3$, are defined as follows:

$$\begin{aligned} g_1(y, x) &= y_1 x^2 + y_2 x + y_3, \\ g_2(y, x) &= y_1 x + y_2, \\ g_3(y, x) &= \sin(y_1 x) + \cos(y_2 x) + y_3. \end{aligned} \quad (2)$$


Figure 4 Trajectories of individual RBCs flowing through a microchannel with the width of 300 μm , around the CFL regions, (a) R_{A300} (b) R_{B300} (c) R_{C300} (d) R_{D300}

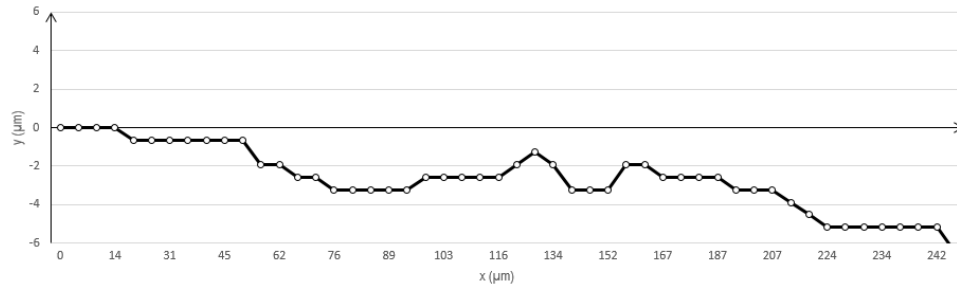


(a)

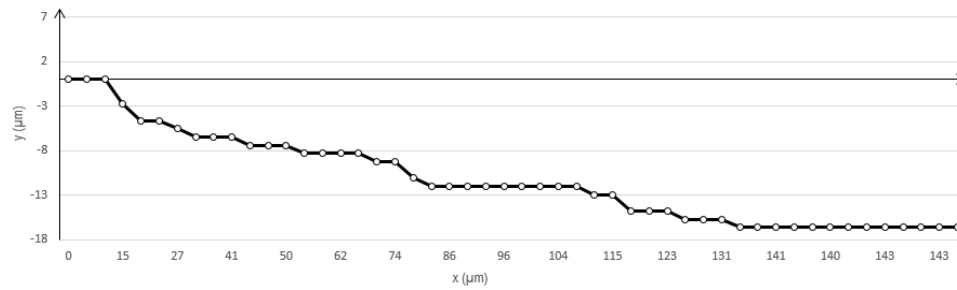

(b)

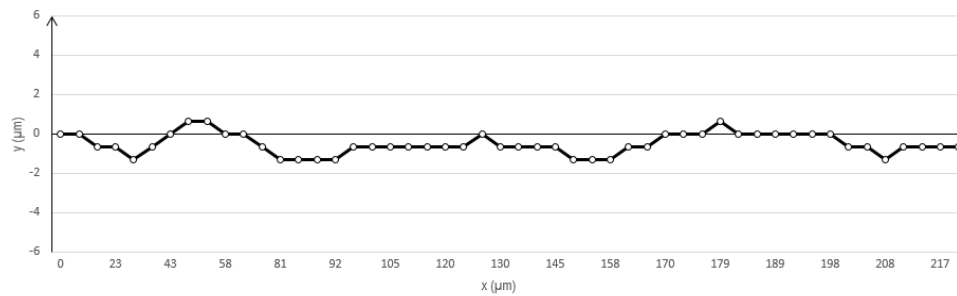


(c)

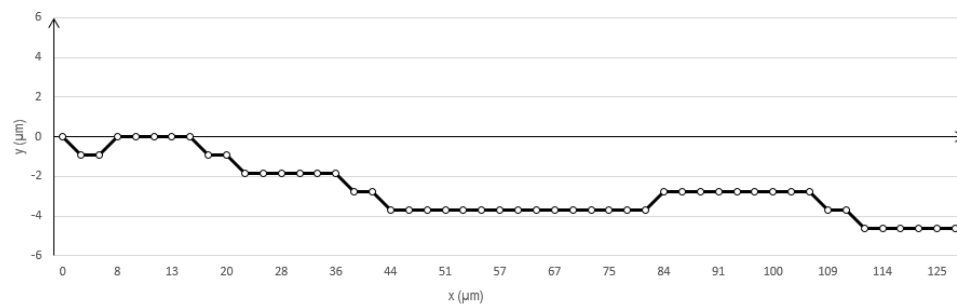


(d)


Figure 5 Trajectories of individual RBCs flowing around the CFL in the microchannel with the width of 500 μm at the regions, (a) R_{A500} (b) R_{B500} (c) R_{C500} (d) R_{D500}

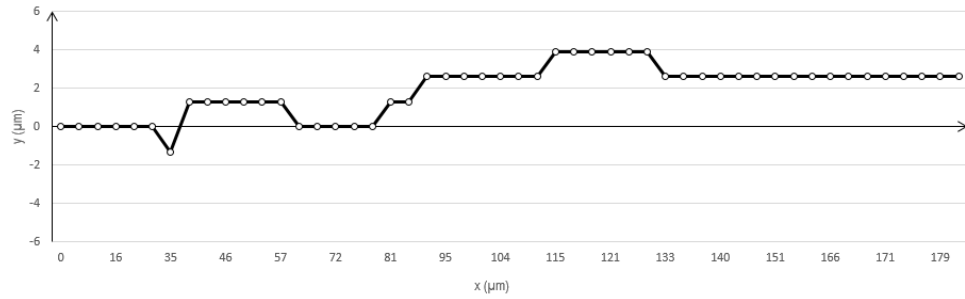


(a)

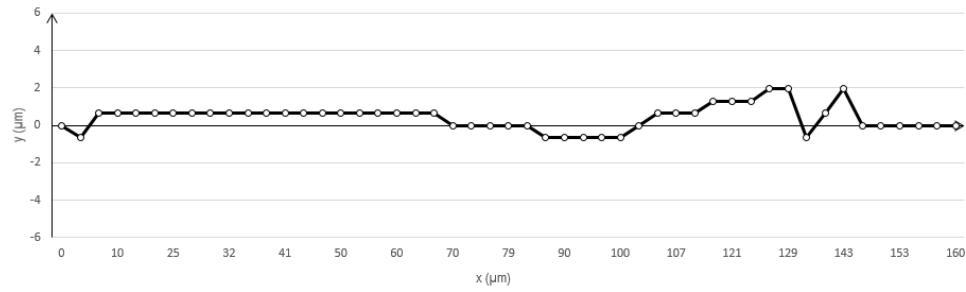

(b)

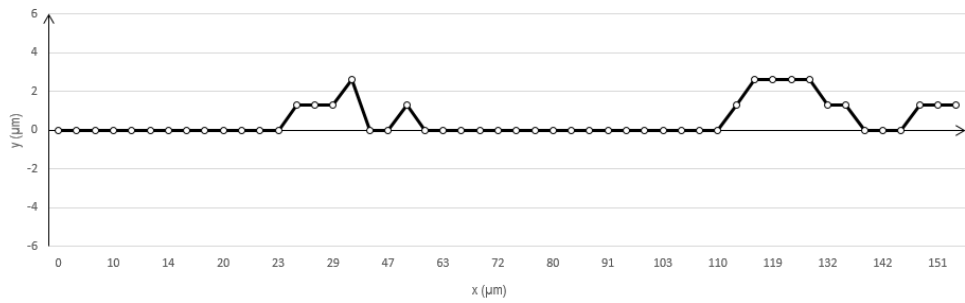


(c)

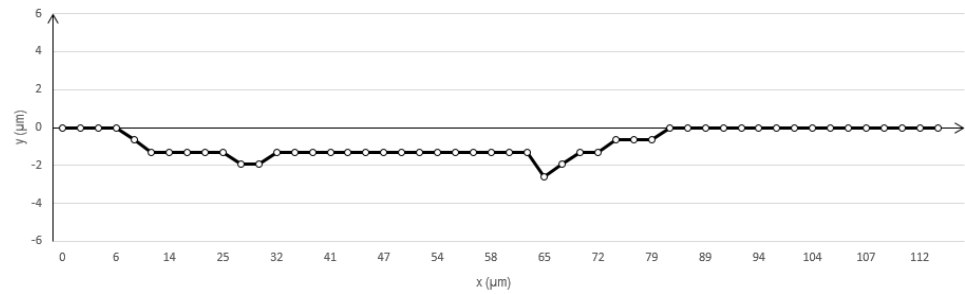


(d)


Figure 6 Trajectories of individual RBCs flowing around the CFL for the regions, (a) R_{A1000} (b) R_{B1000} (c) R_{C1000} (d) R_{D1000}

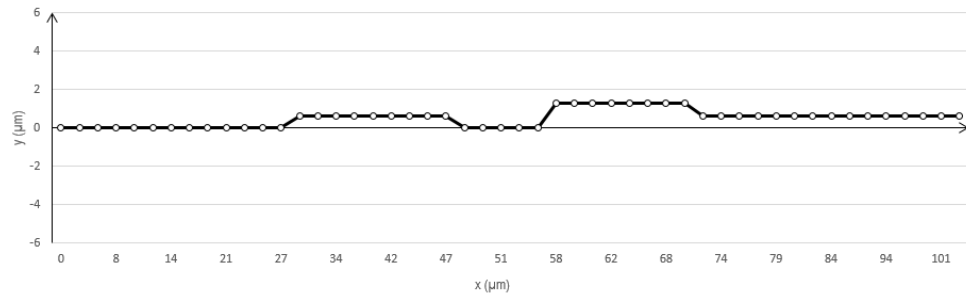


(a)

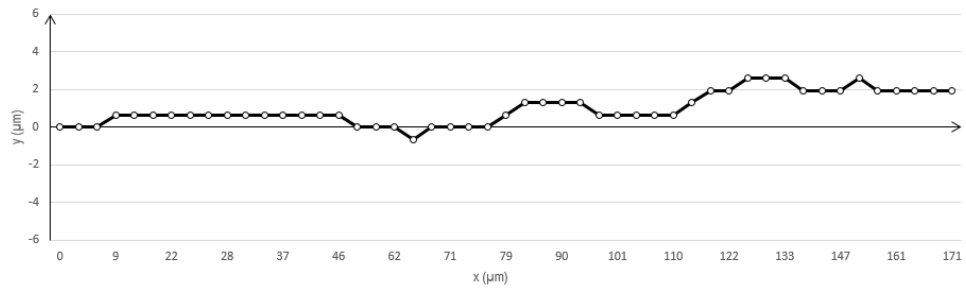

(b)

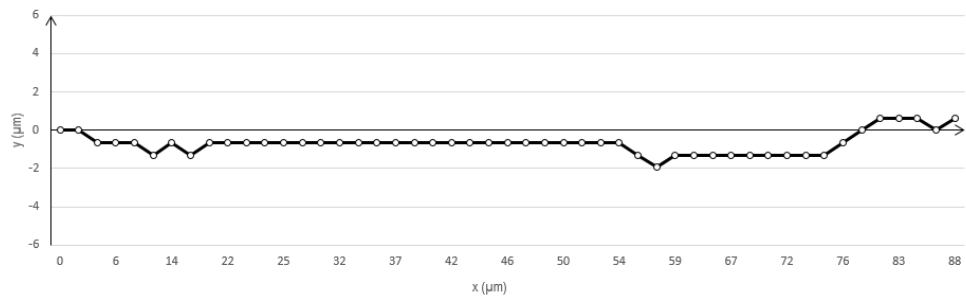

(c)

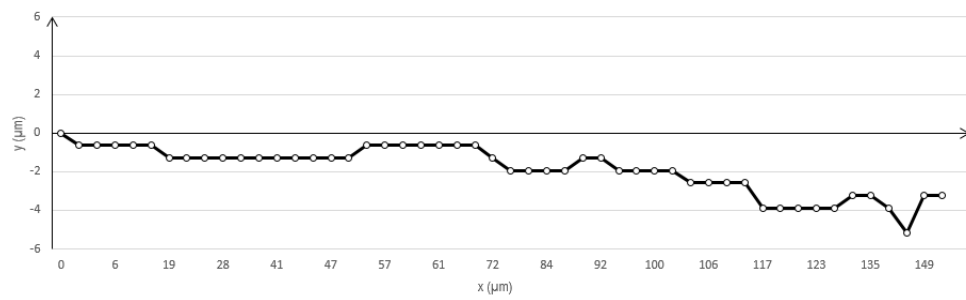

(d)


Table 1 Numerical results obtained using a genetic algorithm

<i>Region</i>	<i>Function</i>	<i>Average</i>	<i>Minimum</i>
R _{A300}	<i>g</i> ₁	4.90E+05	52.18
	<i>g</i> ₂	7.54E+01	31.90
	<i>g</i> ₃	7.39E+01	26.89
R _{A500}	<i>g</i> ₁	1.29E+05	59.82
	<i>g</i> ₂	6.24E+01	38.76
	<i>g</i> ₃	7.00E+01	45.07
R _{A1000}	<i>g</i> ₁	2.00E+04	20.8
	<i>g</i> ₂	1.23E+01	6.46
	<i>g</i> ₃	2.09E+01	8.89
R _{B300}	<i>g</i> ₁	8.94E+04	97.17
	<i>g</i> ₂	6.93E+01	30.42
	<i>g</i> ₃	7.86E+02	621.43
R _{B500}	<i>g</i> ₁	1.37E+05	54.71
	<i>g</i> ₂	3.99E+01	20.63
	<i>g</i> ₃	3.25E+01	19.64
R _{B1000}	<i>g</i> ₁	1.58E+05	50.98
	<i>g</i> ₂	2.73E+01	14.33
	<i>g</i> ₃	3.24E+01	11.09
R _{C300}	<i>g</i> ₁	2.89E+05	42.35
	<i>g</i> ₂	4.88E+01	13.86
	<i>g</i> ₃	2.45E+01	10.50
R _{C500}	<i>g</i> ₁	7.30E+04	57.04
	<i>g</i> ₂	4.66E+01	32.60
	<i>g</i> ₃	3.93E+01	26.63
R _{C1000}	<i>g</i> ₁	1.37E+04	11.36
	<i>g</i> ₂	2.16E+01	14.82
	<i>g</i> ₃	2.06E+01	6.42
R _{D300}	<i>g</i> ₁	4.20E+04	31.76
	<i>g</i> ₂	5.42E+01	35.33
	<i>g</i> ₃	5.23E+01	14.36
R _{D500}	<i>g</i> ₁	2.87E+04	13.32
	<i>g</i> ₂	2.96E+01	19.96
	<i>g</i> ₃	2.18E+01	6.78
R _{D1000}	<i>g</i> ₁	6.92E+04	58.85
	<i>g</i> ₂	4.32E+01	18.71
	<i>g</i> ₃	3.50E+01	13.60


After developing a MatLab code and by applying the genetic algorithm to solve the optimisation problem (1), it was possible to obtain the numerical results shown in Table 1. Since the genetic algorithm is a stochastic method, each problem was solved 100 times. Table 1 presents the regions where the problem (1) was applied, the average of the optimum value and the minimum value obtained in the all 100 runs. The table shows that the minimum value for most of the cases corresponds to the function g_3 .

Figure 7 shows an example of two RBCs trajectories flowing in region R_{A500} and R_{B500} , in a parent microchannel with a width of $500\text{ }\mu\text{m}$, as well as the functions that have revealed a better approximation to the RBCs trajectories.

Figure 7 RBCs trajectories flowing in region (a) R_{A500} and (b) R_{B500} , with a width of $500\text{ }\mu\text{m}$, as well as the functions that have showed a better approximation

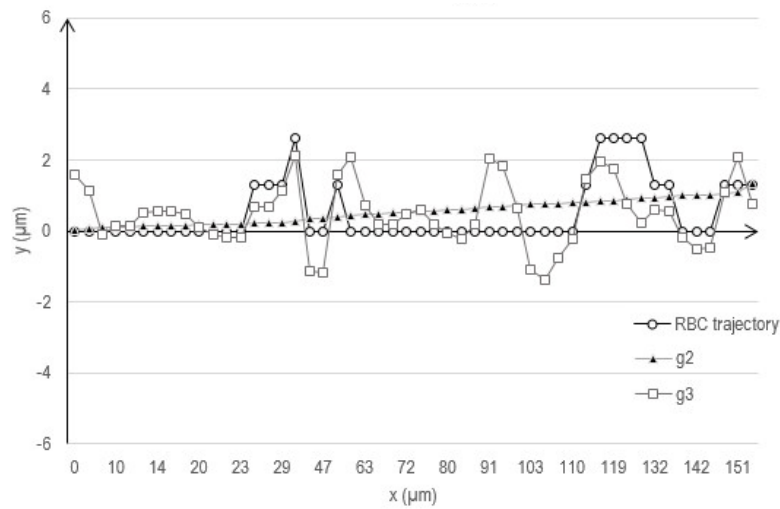

(a)

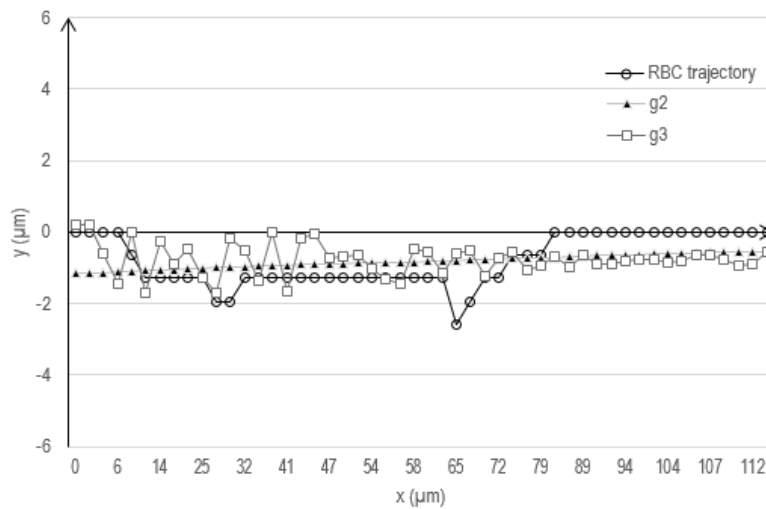

(b)

Function g_1 was not displayed mainly because it was the worst approximation solution to the cells trajectories. Overall, the numerical results suggest that the trigonometric function (g_3) is the one that better resembles the RBCs trajectories and consequently the CFL boundaries, since for the majority of the cases studied the minimum value was obtained for this function. The trigonometric function (g_3) may be due to oscillations caused by collisions between neighbourhood cells flowing around the RBCs core. The only exception was verified in the regions R_{A500} , R_{A1000} , R_{B300} and R_{B1000} (Figures 4, 5, and 6), wherein these regions the best fit was obtained with the function g_2 . Additionally, these results also show that the CFL boundary is size independent and its flow behaviour is not affected by complex geometries such bifurcations and confluences.

4 Conclusions and future directions

In this study, we present a method to measure individual RBCs trajectories flowing around the CFL region. These cells trajectories are believed to closely resemble the CFL boundary and they were fitted using three different functions. A genetic algorithm was used to solve the constrained optimisation problem and the best fit was obtained by using the function (g_3), i.e., a sum of trigonometric functions. This finding corroborates the results obtained by Taboada et al. (2013) and Bento et al. (2015) and where they have performed similar studies in microchannels networks and have found that the function (g_3) is the one that best fit to their CFL measurements. As a future work, we will test other functions and examine a bigger variety of physiological fluids used *in vitro* blood studies.

Acknowledgements

The authors acknowledge the financial support provided by PTDC/SAU-ENB/116929/2010 and EXPL/EMS-SIS/2215/2013 from FCT (Science and Technology Foundation), COMPETE, QREN and European Union (FEDER). R.O. Rodrigues, D. Pinho and V. Faustino acknowledge respectively, the PhD scholarships SFRH/BD/97658/2013, SFRH/BD/89077/2012 and SFRH/BD/99696/2014 granted by FCT.

References

- Bagchi, P. (2007) 'Mesoscale simulation of blood flow in small vessels', *Biophys Journal*, Vol. 92, No. 6, pp.1858–1877.
- Bento, D., Pinho, D., Pereira, A.I. and Lima, R. (2013) 'Genetic algorithm and particle swarm optimization combined with powell method', *Numerical Analysis and Applied Mathematics: AIP Conference Proceedings*, Vols. I–III, No. 1558, pp.578–581.
- Bento, D., Pinho, D., Pereira, A.I. and Lima, R. (2015) 'Cell-free layer measurements in a network with bifurcating microchannels using a global approach', *Operational Research*, pp.53–65, DOI: 10.1007/978-3-319-20328-7_4, Springer International Publishing, Switzerland.
- Caro, C.G., Pedley, T.J., Schroter, R.C. and Seed, W.A. (1978) *The mechanics of the circulation: Second Edition*, Cambridge University Press, New York.

- Catlin, G., Advani, S. and Prasad, A. (2011) 'Optimization of polymer electrolyte membrane fuel cell channels using a genetic algorithm', *Journal of Power Sources*, Vol. 196, No. 2, pp.9407–9418.
- Dupin, M.M., Halliday, I., Care, C.M., Alboul, L. and Munn, L.L. (2007) 'Modeling the flow of dense suspensions of deformable particles in three dimensions', *Phys. Rev. E*, Vol. 75, No. 6, Part 2, 066707.
- Eggleton, C.D. and Popel, A.S. (1998) 'Large deformation of red blood cell ghosts in a simple shear flow', *Physics of Fluids*, Vol. 10, No. 8, pp.1834–1845.
- Faivre, M., Abkarian, M., Bickraj, K. and Stone, H.A. (2006) 'Geometrical focusing of cells in a microfluidic device: an approach to separate blood plasma', *Biorheology*, Vol. 43, No. 2, pp.147–159.
- Faustino, V., Pinho, D., Yaginuma, T., Calhelha, R., Ferreira, I. and Lima, R. (2014) 'Extensional flow-based microfluidic device: deformability assessment of red blood cells in contact with tumor cells', *BioChip Journal*, Vol. 8, No. 1, pp.42–47.
- Fedosov, D.A., Caswell, B., Popel, A.S. and Karniadakis, G. (2010) 'Blood flow and cell-free layer in microvessels', *Microcirculation*, Vol. 17, No. 8, pp.615–628.
- Gambaruto, A.M. (2015) 'Computational haemodynamics of small vessels using the moving particle semi-implicit (MPS) method', *Journal of Computational Physics*, Vol. 302, No. 1, pp.68–96.
- Garcia, V., Dias, R. and Lima, R. (2012) 'In vitro blood flow behaviour in microchannels with simple and complex geometries', in Naik, G.R. (Ed.): *Applied Biological Engineering – Principles and Practice*, pp.393–416, ISBN: 978-953-51-0412-4, InTech, Croatia.
- Goldsmith, H. and Turitto, V. (1986) *Rheological Aspects of Thrombosis and Haemostasis: Basic Principles and Applications*, ICTH-Report-Subcommittee on Rheology of the International Committee on Thrombosis and Haemostasis, Thromb Haemost, Vol. 55, pp.415–435.
- Holland, J.H. (1975) *Adaptation in Natural and Artificial Systems*, The University of Michigan Press, Ann Arbor.
- Imai, Y., Kondo, H., Ishikawa, T., Lim, C.T. and Ymaguchi, T. (2010) 'Modeling of hemodynamics arising from malaria infection', *Journal of Biomechanics*, Vol. 43, No. 7, pp.1386–1393.
- Kim, S., Kai Ong, P., Yalcin, O., Intaglietta, M. and Johnson, P.C. (2009) 'The cell-free layer in microvascular blood flow', *Biorheology*, Vol. 46, No. 3, pp.181–189.
- Kumar, M., Husian, M., Upreti, N. and Gupta, D. (2010) 'Genetic algorithm: review and application', *International Journal of Information Technology and Knowledge Management*, Vol. 2, No. 2, pp.451–454.
- Leble, V., Lima, R., Dias, R., Fernandes, C., Ishikawa, T., Imai, Y. and Yamaguchi, T. (2011) 'Asymmetry of red blood cell motions in a microchannel with a diverging and converging bifurcation', *Biomicrofluidics*, Vol. 5, No. 4, pp.044120-1–15.
- Lima, R., Ishikawa, T., Imai, Y. and Yamaguchi, T. (2012) 'Blood flow behavior in microchannels: advances and future trends', in Dias, R., Martins, A.A., Lima, R. and Mata, T.M. (Eds.): *Single and Two-Phase Flows on Chemical and Biomedical Engineering*, pp.513–547, Bentham Science, Beijing, China.
- Lima, R., Ishikawa, T., Imai, Y., Takeda, M., Wada, S. and Yamaguchi, T. (2008) 'Radial dispersion of red blood cells in blood flowing through glass capillaries: role of hematocrit and geometry', *Biomechanics Journal*, Vol. 44, No. 10, pp.2188–2196.
- Lima, R., Ishikawa, T., Imai, Y., Takeda, M., Wada, S. and Yamaguchi, T. (2009a) 'Measurement of individual red blood cell motions under high hematocrit conditions using a confocal micro-PTV system', *Annals of Biomedical Engineering*, Vol. 37, No. 8, pp.1546–1559.
- Lima, R., Nakamura, M., Omori, T., Ishikawa, T., Wada, S. and Yamaguchi, T. (2009b) 'Microscale flow dynamics of red blood cells in microchannels: an experimental and numerical analysis', in Tavares, J.M. and Jorge, R.M. (Eds.): *Computational Vision and Medical Processing: Recent Trends*, pp.203–220, Springer International Publishing, Switzerland.

- Lima, R., Wada, S., Tsubota, K. and Yamaguchi, T. (2006) 'Confocal micro-PIV measurements of three dimensional profiles of cell suspension flow in a square microchannel', *Measurement Science and Technology*, Vol. 17, No. 4, pp.797–808.
- Liu, W.K., Liu, Y., Farrell, D., Zhang, L., Wang, S.X., Fukui, Y., Patankar, N., Zang, Y., Bajaj, C., Lee, J., Hong, J., Chen, X. and Hsu, H. (2006) 'Immersed finite element method and its applications to biological systems', *Computer Methods in Applied Mechanics and Engineering*, Vol. 195, Nos. 13–16, pp.1722–1749.
- Maeda, N. (1996) 'Erythrocyte rheology in microcirculation', *Japanese Journal of Physiology*, Vol. 46, No. 1, pp.1–14.
- Nakamura, M., Bessho, S. and Wada, S. (2013) 'Spring-network-based model of a red blood cell for simulating mesoscopic blood flow', *International Journal for Numerical Methods in Biomedical Engineering*, Vol. 29, No. 1, pp.114–128.
- Omori, T., Ishikawa, T., Barthès-Biesel, D., Salsac, A.V., Walter, J., Imai, Y. and Yamaguchi, T. (2011) 'Comparison between spring network models and continuum constitutive laws: application to the large deformation of a capsule in shear flow', *Physical Review*, Vol. 83, No. 4, pp.041918-1–11.
- Pinho, D., Gayubo, F., Pereira, A.I. and Lima, R. (2013a) 'A comparison between a manual and automatic method to characterize red blood cell trajectories', *International Journal for Numerical Methods in Biomedical Engineering*, Vol. 29, No. 9, pp.977–987.
- Pinho, D., Yaginuma, T. and Lima, R. (2013b) 'A microfluidic device for partial cell separation and deformability assessment', *BioChip Journal*, Vol. 7, No. 4, pp.367–374.
- Pinto, E., Faustino, V., Rodrigues, R., Pinho, D., Garcia, V., Miranda, J. and Lima, R. (2015) 'A rapid and low-cost nonlithographic method to fabricate biomedical microdevices for blood flow analysis', *Micromachines*, Vol. 6, No. 1, pp.121–135, DOI: 10.3390/mi6010121.
- Pries, A. and Secomb, T. (1994) 'Resistance to blood flow in microvessels in vivo', *Circulation Research*, Vol. 75, No. 5, pp.904–915.
- Rodrigues, R., Faustino, V., Pinto, E., Pinho, D. and Lima, R. (2014) 'Red blood cells deformability index assessment in a hyperbolic microchannel: the diamide and glutaraldehyde effect', *WebmedCentralplus Biomedical Engineering*, Vol. 1, pp.WMCPLS00253-1–6.
- Sollier, E., Cubizolles, M., Fouillet, Y. and Achard, J.L. (2010) 'Fast and continuous plasma extraction from whole human blood based on expanding cell-free layer devices', *Biomedical Microdevices*, Vol. 12, No. 3, pp.485–497.
- Suzuki, Y., Tateishi, N., Soutani, M. and Maeda, N. (1996) 'Deformation of erythrocytes in microvessels and glass capillaries: effects of erythrocyte deformability', *Microcirculation*, Vol. 3, No. 1, pp.49–57.
- Taboada, B., Bento, B., Pinho, D., Pereira, A.I. and Lima, R. (2013) 'Cell-free layer measurements in bifurcating microchannels: a global approach', *Proceedings of IO 2013*, pp.341–346.
- Tsubota, K., Wada, S. and Yamaguchi, T. (2006a) 'Particle method for computer simulation of red blood cell motion in blood flow', *Computer Methods and Programs in Biomedicine*, Vol. 83, No. 2, pp.139–146.
- Tsubota, K., Wada, S., Kamada, H., Lima, R. and Yamaguchi, T. (2006b) 'A particle method for blood flow simulation – application to flowing red blood cells and platelets', *Journal of the Earth Simulator*, Vol. 5, No. 1, pp.2–7.
- Yaginuma, T., Oliveira, M.S.N., Lima, R., Ishikawa, T. and Yamaguchi, T. (2013) 'Human red blood cell behavior under homogeneous extensional flow in a hyperbolic-shaped microchannel', *Biomicrofluidics*, Vol. 7, No. 5, 054110 [online] <http://dx.doi.org/10.1063/1.4820414> (accessed October 2015).
- Yamaguchi, T., Ishikawa, T., Tsubota, K., Imai, Y., Nakamura, M. and Fukui, T. (2006) 'Computational blood flow analysis – new trends and methods', *Journal of Biomechanical Science and Engineering*, Vol. 1, No. 1, pp.29–50.